

ZEPPEL CLARITY **Pixie**

OTC Hearing Aids

User Guide

Warnings



Warning: If you are younger than 18, do not use this.

You should go to a doctor, preferably an ear-nose-throat doctor (an ENT), because your condition needs specialized care. Over-the-counter hearing aids are only for users who are age 18 or older.

This OTC hearing aid is for users who are 18 and older. People who are younger than 18 with hearing loss should see a doctor, preferably an ENT, because they may need medical testing and management. Hearing loss can affect speech and learning, so professional fitting and continuing care are also important.




Warning: When to see a doctor

If you have any of the problems listed below, please see a doctor, preferably an ear-nose-throat doctor (an ENT).

- Your ear has a birth defect or an unusual shape. Your ear was injured or deformed in an accident.
- You saw blood, pus, or fluid coming out of your ear in the past 6 months
- You have a lot of ear wax, or you think something could be in your ear
- You get really dizzy or have a feeling of spinning or swaying (called vertigo)
- Your hearing changed suddenly in the past 6 months

- Your hearing changes: it gets worse then gets better again
- You have worse hearing in one ear
- You hear ringing or buzzing in only one ear

 **Warning: This hearing aid should not cause pain when inserting it.**

Remove this device from your ear if it causes pain or discomfort when you insert or place it. To try again, make sure to follow the instructions. If you feel pain or discomfort again, contact the manufacturer. If your pain or discomfort doesn't go away, contact your hearing healthcare professional. You can also report this to FDA as an adverse event according to the instructions that appear later.

 **Warnings:**

- Keep and store hearing aids and components out of reach of children. Contains small parts which may be a choking hazard.
- Check before using the hearing aids in areas where electronics or wireless devices are restricted. This may cause interference.
- Do **NOT** dry hearing aid with a hairdryer. Heat may damage hearing aid.
- Do **NOT** use the hearing aids without the supplied ear tips attached.

- Do **NOT** use the hearing aids in explosive or oxygen-enriched atmospheres. Otherwise, a fire or explosion could occur.
- Do **NOT** resell the hearing aids or share them with others. They are intended for use by a single user. Using resold or shared hearing aids may lead to infection.
- Do **NOT** submerge in water, wear in the shower, or wear while participating in water sports, e.g., swimming, waterskiing, surfing, etc. Prolonged exposure to water may damage the hearing aids.
- Do **NOT** repair or replace the lithium-ion rechargeable battery yourself. Contact us if you believe a battery replacement is required.
- Do **NOT** insert hearing aids into the ear canal while sleeping.
- Do **NOT** use hearing aids during X-rays, MRIs, CT scans or other similar medical treatment to prevent damage to the hearing aid.
- Do **NOT** expose hearing aid to contaminants such as hair spray, mousse, gel, lotions, etc. to prevent damage to the hearing aid.
- Do **NOT** use an instrument, such as a cotton swab, to push the hearing aid in the ear canal. Hearing aids may be placed too deep and cause damage to the ear.
- Do **NOT** place charging case in clothing pocket while charging with the USB power cable. The charging case may overheat and malfunction.

Cautions



Caution: This is not hearing protection.

You should remove this device if you experience overly loud sounds, whether short or long-lasting. If you're in a loud place, you should use the right kind of hearing protection instead of wearing this device. In general, if you would use ear plugs in a loud place, you should remove this device and use ear plugs.



Caution: The sound output should not be uncomfortable or painful.

You should turn down the volume or remove the device if the sound output is uncomfortably loud or painful. If you consistently need to turn the volume down, you may need to further adjust your device.



Caution: You might need medical help if a piece gets stuck in your ear.

If any part of your hearing aid, like the eartip, gets stuck in your ear, and you can't easily remove it with your fingers, get medical help as soon as you can. You should not try to use tweezers or cotton swabs because they can push the part farther into your ear, injuring your eardrum or ear canal, possibly seriously.

Notes

! Note: If you remain concerned, consult a professional.

If you try this device and continue to struggle with or remain concerned about your hearing, you should consult with a hearing healthcare professional.

! Note: What you might expect when you start using a hearing aid

A hearing aid can benefit many people with hearing loss. However, you should know it will not restore normal hearing, and you may still have some difficulty hearing over noise. Further, a hearing aid will not prevent or improve a medical condition that causes hearing loss.

People who start using hearing aids sometimes need a few weeks to get used to them. Similarly, many people find that training or counseling can help them get more out of their devices.

If you have hearing loss in both ears, you might get more out of using hearing aids in both, especially in situations that make you tired from listening—for example, noisy environments.

! Note: Tell FDA about injuries, malfunctions, or other adverse events.

To report a problem involving your hearing aid, you should submit information to FDA as soon as possible after the problem. FDA calls them "adverse events," and they might include: skin irritation in your ear, injury from the device (like

cuts or scratches, or burns from an overheated battery), pieces of the device getting stuck in your ear, suddenly worsening hearing loss from using the device, etc.

Instructions for reporting are available at <https://www.fda.gov/Safety/MedWatch>, or call 1-800-FDA-1088. You can also download a form to mail to FDA.



Cautions:

- Do **NOT** use the hearing aids or their components if any part of them is damaged, if they emit any loud unusual noise, if you experience a warming sensation, or if you experience loss of audio.
- Do **NOT** make unauthorized alterations to this product.
- Only use attachments/components specified by the manufacturer.
- Avoid using ear tips, adapters, cables, and other accessories not specified or provided by the manufacturer as it could result in increased electromagnetic emissions or decreased electromagnetic immunity of the hearing aids as well as improper operation.
- Avoid use of hearing aid systems directly next to other electronic equipment, which could result in decreased performance. If such use is necessary, monitor the performance of your hearing aid system and the other equipment to ensure they are operating normally.
- If the battery leaks, do **NOT** allow the liquid to come in contact with the skin or eyes. If contact made, seek medical advice.

- Keep hearing aids away from fire and excessive heat (e.g., from storage in direct sunlight, near candles, or in a hot car) to avoid burns or damage to product.
- Be aware that some sounds may sound different when you're using the hearing aids. Keep this in mind when you need to be aware of your surroundings. You should adjust to this over time.
- Consult a hearing care professional, preferably an ear-nose-throat doctor (ENT) if you experience any unusual side effects like skin irritation, excessive accumulation of ear wax, dizziness, change in your hearing, or if you think there may be a foreign object in your ear canal.

Content

Intended Use	01
Indications for Use	01
Your Hearing Aids	02
What's in the Box	02
Overview	04
Download the Zepp Clarity App	05
Daily Use	06
Charging the Hearing Aids	06
Hearing Aids Instructions	07
Charge the Charging Case	08
Charging Case Instructions	09
Inserting the Hearing Aids	10
Removing the Hearing Aids	12
Find the Most Suitable Dome	13
The Size of Dome	14
Zepp Clarity App	15
Program Recommendation	15
Adjusting Volume	16
Mute	17
Checking the Battery Level	17
Switching the Hearing Program	18
Clarity Boost	20
Smart Phonecall	21

Care and Maintenance	22
Daily Care	22
Remove the Dome	23
Replace the Mic Caps	25
Technical Information	27
Troubleshooting	29
Further Information	31
Operating, Transport & Storage Conditions	31
Safety Information	31
Waste Disposal	33
Compliance Information	33
Wireless Technical Description	36
Symbols and Descriptions	37
Warranty and Service	39
Repair	39
Exclusions from Warranty Repair Coverage	40
Loss and Damage	42

Intended Use

The Zepp Clarity Pixie hearing aids are a pair of OTC wireless air conduction hearing aids intended for use by individuals 18 years and older with perceived mild to moderate hearing impairment.

Indications for Use

The Zepp Clarity Pixie hearing aids are intended to amplify sound for individuals 18 years of age or older with perceived mild to moderate hearing impairment. No programming or user-fitted is necessary. The device is intended for over-the-counter sale and use without the assistance of a hearing care professional.

Your Hearing Aids

What's in the Box



**2 Zepp Clarity Pixie
Hearing Aids***



Charging Case



2 Size S Open Domes



2 Size S Closed Domes



2 Size M Open Domes



2 Size M Closed Domes



**2 Replaceable
Mic Cap**

*Size M Open Domes are pre-attached to the devices.



**USB
Power Adapter**



**USB-C
Power Cable**



Cleaning Cloth



Cleaning Brush





User Guide



Quick Start Guide

Overview

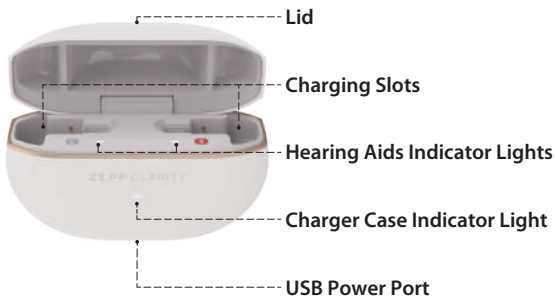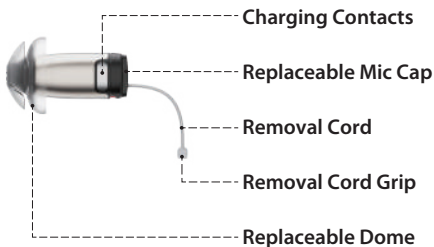

Download the Zepp Clarity App

With the Zepp Clarity App, you can customize your hearing aids to suit your preferences. You can adjust the volume, change the hearing programs, locate your hearing aids, update the firmware, and more.

To get the app, go to the Apple App Store or Google Play Store on your smartphone and search for Zepp Clarity. Or, you can scan the QR code below with your smartphone's camera and download it directly.



Daily Use

Charging the Hearing Aids

Place the right hearing aid in the charging slot marked with a "R", and the left one in the slot with a "L". Make sure the domes are pointing outwards, and the removal cord is pointing upwards. Gently press down on the hearing aids with your thumb or index finger to make sure they are properly placed in the charging slots.



Hearing Aids Instructions



White light: Hearing aids are correctly placed and have sufficient battery.



Orange light: Hearing aid have insufficient battery and are charging.



Indicator light off: Hearing aids are not properly placed or charging case is out of power. Please place the hearing aid again or charge the charging case.

*Indicator lights time out after about 15 seconds.

Charge the Charging Case

- Charge the charging case by connecting to the provided USB-C Power Cable and USB Power Adaptor or by using a Qi wireless charging pad*.
- It takes about 2.5 hours to fully charge the charging case by using power socket.



*Qi wireless charging pad is not included and needs to be purchased separately.

Charging Case Instructions



White light: The charging case battery is sufficient.



Orange light: The charging case battery is low or charging.




Indicator light off*: Charging case is out of power. Please charge the charging case.

*The charging case indicator light will only illuminate when you open the lid or connect the power adapter.

Inserting the Hearing Aids




Remove the hearing aids from the charging case and check the markings. The letter 'L' indicates the left ear, while 'R' indicates the right ear.



Gently insert the hearing aid into your ear.



Slowly push the hearing aid into place. The black Mic Cap should rest at your ear canal opening. If the device feels loose in your ear, see page 14 to learn how to choose the right dome size.



For most ears, the Removal Cord Grip should be in this position. If the Removal Cord Grip rests more deeply in your ear, grasp it and pull the device out a bit.

Removing the Hearing Aids



Pinch the Removal Cord Grip with your thumb and index finger and gently pull outwards to remove the hearing aids from the ear canal.



Wipe the device gently with the Cleaning Cloth. Placing them into the Charging Case.

Find the Most Suitable Dome


Zepp Clarity Pixie ship with open and closed domes, each in S and M sizes. If the domes don't feel comfortable or secure, choose another dome size.

Open Dome



The Open Dome have two layers of blades, each with three openings. This design make your voice sound more natural.

Closed Dome



Closed Dome consists of two layers of blades, each with two openings. This design provide more bass, and can also be effective at eliminating feedback noise.

The Size of Dome

Once you have chosen the type of domes, the next step is to choose the right size. Ideal domes should be slightly larger than the ear canals but exert no extra pressure.

If your domes are too small, they cannot stay fixed in the ear canals and cannot provide the standard sound quality and volume. If your domes are too large, they may get stuck in your ear canals and may cause pain inside your ears.



Some people have left and right ear canals that are not the same size, and if this is the case for you, you may need to use a M-sized dome for one ear and a S-sized dome for the other. Don't worry, this is very common. Besides, we recommend that you wear the domes for at least one hour to decide which dome suits you best. During this time, you can try having conversations, eating, drinking, exercising, etc. This may help you select the dome that provides maximum comfort throughout the day.

Zepp Clarity App

Program Recommendation


If you are using Zepp Clarity Pixie hearing aids for the first time, we highly recommend that you use the program recommendation feature. This feature can recommend one of three standardized output profiles for you based on your hearing impairment situation, and automatically set the volume, which will significantly improve your hearing experience.

Please run this feature in a relatively quiet room. The whole process may take 3-5 minutes.

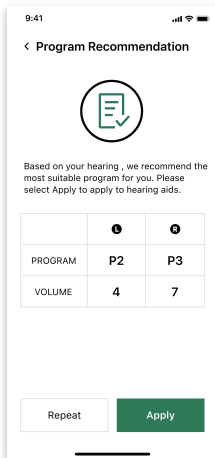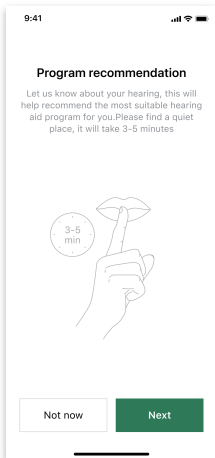

Adjusting Volume

You can adjust the volume of your hearing aids with the Zepp Clarity App:


- You can swipe the volume bar upwards or downwards to adjust the volume of your hearing aids.
- Tap the button  in the middle, you can adjust the volume of the Left and Right ear separately.



Mute

The mute feature enables you to hear sounds like you're not wearing hearing aids. Perform the following operations on the home screen of the Zepp Clarity App:

Tap the mute button  under the volume bar.

If you want to unmute, tap the mute button  again.

Checking the Battery Level


At the top of the home screen of the Zepp Clarity App, you can check the battery level of the hearing aids and the charging case.


 indicates the available battery percentage.

 indicates charging.


Switching the Hearing Program

The hearing aids support 8 preset hearing programs for you to choose freely in different scenarios.

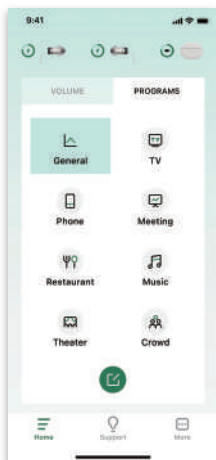

By tapping the edit button  below the preset hearing program, you can customize the preset hearing program according to your own needs:


- Adjust pitches (Bass, Middle, Treble);
- Adjust noise cancellation depth.

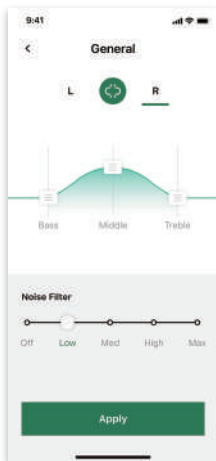

Clarity Boost

This feature can help you make conversations more easily. You can be enabled on the "More" page at the bottom of the home screen of the Zepp Clarity App.

Quickly double tap your ear to turn this feature on or off. Please note that the requires you to operate separately on each ear separately.


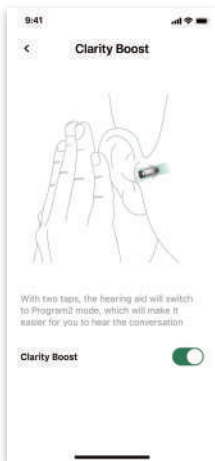


Smart Phonecall

This feature can be enabled on the "More" page at the bottom of the home screen of the Zepp Clarity App.

After this feature is enabled, your hearing aids will play a tone as a reminder when there is an incoming call.

Meanwhile, the hearing aids automatically switch to "Phone" mode during a call, which effectively avoids the feedback of the hearing aids when you're on a phonecall, and makes it easier for you to listen to the call.

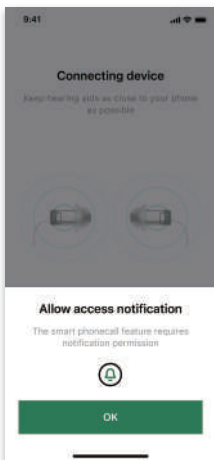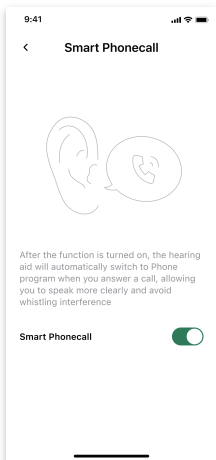

Care and Maintenance

With daily use, please clean your hearing aids each day to avoid dirt buildup which could cause degradation, damage, or an ear canal allergic reaction.

Daily Care



Brush the Dome to remove wax and debris.



Brush around the Mic Cap to remove wax and debris.



Wipe the main body with the Cleaning Cloth.

Replace the Dome



Pinch the body of the hearing aids firmly with your thumb and index finger, then use your other hand to grab the dome and remove it.



Brush the sound outlet to remove wax and debris.



Select a new Dome. Align the sound outlet with the center of the new Dome.



Press into place until you feel a click.

Replace the Mic Caps




Insert the crowbar at the end of the Cleaning Brush into the orange/grey marked groove at the end of the hearing aids.




Gently pry the Mic Cap off the hearing aids. Gently pinch the Mic Cap with the other hand and pull it through the removal cord and remove it.



Use a Cleaning Brush to gently brush off the ear wax and skin debris on the Mic Cap, and then use a wipe to clean the oil and sweat around the microphone opening.



Take a new Mic Cap.



Pass the circular hole on the Mic Cap through the Removal Cord Grip.



Attach the Mic Cap to the hearing aids, you will hear the sound of clicks.

Technical Information

Measurements per ANSI/CTA2051:2017	Result	
Maximum output (OSPL90)	110 dB SPL	
Maximum output (OSPL90) curve	See Figure 1	
High-frequency average (HFA) OSPL90	106 dB SPL	
Average full-on gain (HFA-FOG)	31 dB	
Reference test gain	28 dB	
Frequency response bandwidth / range	200 – 7500 Hz	
Frequency response curve	See Figure 2	
Total harmonic distortion	500 Hz @70 dB	0.9%
	800 Hz @70 dB	0.7%
	1600 Hz @65 dB	0.5%
Total harmonic distortion + noise	500 Hz @70 dB	4.5%
	500 Hz @100 dB	1.5%
Equivalent input noise (noise reduction disabled)	26 dB SPL	
Equivalent input noise (noise reduction enable)	13 dB SPL	
Latency	6 ms	
Power supply specification	Input: 100-240V~ 50/60 Hz, 0.4A Output: 5V, 1A	
Battery current drain (hearing aid)	530µA max current	
Working time	17 hours	

Figure 1: Nominal OSPL90 curve as measured in a 2 cc coupler.


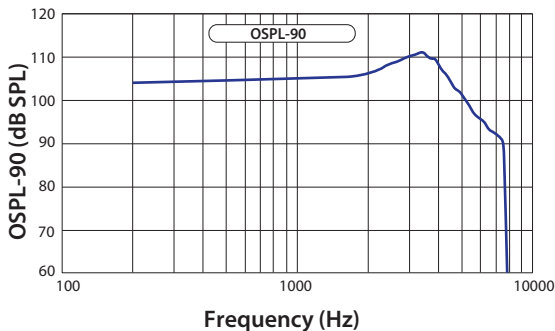


Figure 2: Nominal frequency response curve as measured in a 2 cc coupler.

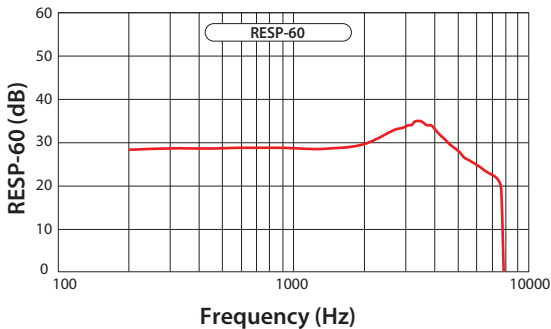

Troubleshooting

Issue	Solutions
No Sound.	<ol style="list-style-type: none">1. Ensure hearing aids and charging case are charged.2. Change or clean dome.3. Change or clean microphone cover.
Too soft / sound quality seems low, weak or diminished.	<ol style="list-style-type: none">1. Use the Clarity App to change volume in programs.2. Change or clean dome.3. Change or clean mic cap.
Too loud.	<ol style="list-style-type: none">1. Use the Clarity App to change volume in programs.
Different volumes in right and left ear.	<ol style="list-style-type: none">1. Use the Clarity App to change volume in programs.
Hearing aids whistle, ring or buzz.	<ol style="list-style-type: none">1. Try the closed dome style, or choose a larger size dome.2. Sound inlet too close to another object (e.g., a phone); ensure there is space around the sound inlet.
No Lights on charging case.	<ol style="list-style-type: none">1. Ensure hearing aids and charging case are charged.2. Open / closed charging case Lid.

Issue	Solutions
Dome remains in ear.	1. Have the item removed from your ear by a healthcare professional. Do NOT attempt to remove the item yourself.
Mic cap remains in ear.	1. Have the item removed from your ear by a healthcare professional. Do NOT attempt to remove the item yourself.
Physical fit not as expected.	<ol style="list-style-type: none"> 1. Change or clean dome. 2. Try different dome types and sizes. 3. Ensure hearing aid is correctly inserted.
Cannot adapt to hearing amplified sound (e.g., own voice too loud, background sounds audible, etc.).	1. Get help from a customer service advisor. Dial (855) 619-4327 to contact us.
Hearing aids will not turn off.	<ol style="list-style-type: none"> 1. Clean hearing aids, Cradles on charging case with cleaning brush / cloth. 2. Ensure correct orientation and placement in charging case.
Hearing aids does not work.	1. Ensure hearing aids and charging case are charged.

Further Information

Operating, Transport & Storage Conditions

Operating conditions	Temperature	Relative humidity	Atmospheric pressure
Operating	5 to 40 °C (41 to 104 °F)	0 to 90 %	700 to 1060 hPa
Storage	-20 to 50 °C (-4 to 122 °F)	0 to 90 %	700 to 1060 hPa
Transport	-20 to 50 °C (-4 to 122 °F)	0 to 90 %	700 to 1060 hPa

Safety Information



Warning

- A lithium-ion rechargeable battery is permanently built into your hearing aid. Incorrect use of the hearing aid can cause the lithium-ion rechargeable battery to burst, risk of injury, fire or explosion!
- Expected battery life: 2 Years
- Follow the safety instructions for lithium-ion rechargeable battery in this section.
- Keep out of reach of children and pets.

- Observe the operating conditions. Refer to the section "Operating, transport, and storage conditions".
- Check your medications before taking them— hearing aids have been mistaken for pills.
- Pay special attention to protect your aid from extreme heat (e.g., fire, microwave oven, induction oven or other high induction fields) and sunlight.
- Never put hearing aids in your mouth, as they can easily be swallowed.
- Charge your hearing aids only with the approved charging case and cable.
- Do **NOT** disassemble your hearing aids.
- Do **NOT** use hearing aids in explosive atmospheres.
- Do **NOT** use deformed or visibly damaged hearing aids.
- Possible physiological side effects: please contact us if you develop skin irritation or accelerated ear wax buildup.



Waste Disposal

The hearing aids, charging case, USB-C power cable, and USB-C power cable must be recycled at an e-waste facility or sent back to Zepp. Everything else goes in normal waste.

FCC Compliance Information

This device complies with FCC 47 CFR Part 15, subpart C.

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

Changes or modifications not expressly approved by Huami could void the user's authority to operate this equipment.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions:

1. This device may not cause harmful interference, and
2. this device must accept any interference received, including interference that may cause undesired operation.

This device complies with FCC radiation exposure limits set forth for general population. This transmitter must not be co-located or operating in conjunction with any other antenna or transmitter.

FCC ID: 2AC8UA2285

Hearing Aid Model: A2285

Charging Case Model: A2207Y

Radio Transceiver Frequency Range: 2.4 to 2.4835 GHz

Radio Receiver Bandwidth: 2 MHz

Modulation Type: 1 Mb/s

GFSK Peak Effective Isotropic Radiated Power: 0 dBm

Antenna Type: Monopole antenna

Modulation: GFSK

Radiated Power: < 1mW

Range: < 10m

Wireless Technical Description

Classification: Your Zepp Clarity Pixie hearing aid is classified as Class II exempt per 21 CFR 874 and Type B per IEC 60601-2-66.

This hearing aid model has been tested to, and has passed, the following EMC, emissions, and immunity tests:

- IEC 60601-1-2 radiated emissions requirements for a Group 1, Class B device as stated in CISPR 11.
- Immunity to ESD levels of +/- 8 kV conducted discharge and +/-15 kV air discharge.

Symbols and Descriptions



Warning/Caution: Important information for injury prevention, handling, and product safety.



Consult instructions for use.



Note.



Keep magnets away from hearing aids to avoid damage.



Relative humidity: Store between 0% to 90% relative humidity.



Atmospheric pressure should be 700 hPa to 1060 hPa.



Contains electronics, dispose according to local regulations, or return to the manufacturer.



Do **NOT** use if package is damaged.



Bluetooth[®] low energy technology.



Manufacturer.



Date of manufacture.



Catalogue number.



Type B applied part.



Serial number.

Warranty and Service

45-day right to return: Zepp Clarity Pixie grants you a 45-day right to return starting from the date of delivery. To receive a return authorization, please contact our customer support team at (855)619-4327. If you are not satisfied with your Zepp Clarity hearing aids, you have the option of returning the device within forty-five (45) days after delivery. As long as the device is in its original condition and has not been damaged, lost or modified (including repaired without our prior written consent) in any way, we will credit back the purchase price to the account used at the time of purchase, less any expedited shipping if any.

Warranty period: Zepp Clarity Pixie offers you a two-year limited warranty valid starting from the date of delivery.

Repair

What your warranty policy covers: This limited warranty covers defects in material and workmanship for the Zepp Clarity Pixie hearing aids, which includes the hearing aids, internal components, and charger within the limited warranty period. This warranty is guaranteed by Zepp North America, Inc.

Number of repairs: Unlimited during warranty period for repairs covered by warranty terms.

What you get with your repair: For valid repairs, Zepp Clarity pledges to secure functionality at least equivalent to the original hearing aid. At the discretion of Zepp Clarity, hearing aids may be replaced by new products or products manufactured from new or serviceable used parts or repaired using new or refurbished replacement parts.

Exclusions from Warranty Repair Coverage

- Normal wear and tear.
- Cosmetic damage, including but not limited to scratches, dents, and broken plastic on ports unless failure has occurred due to a defect in materials or workmanship.
- Defects or damage caused by misuse, accident (including without limitation collision, fire, flood, earthquake and the spillage of food or liquid), neglect, abuse, alteration, unusual stress, modification, improper or unauthorized repair, installation, wiring, or testing, improper storage, use with unsuitable devices, software, or services.

- Use not in accordance with the technical specification of the product.
- Damage caused by third party equipment with which the product is used.
- Commercial use or resale.
- Features or performance parameters pertaining to any software or services beyond the product's normal use function substantially in accordance with Zepp's technical specifications or accompanying product documentation.
- A product that is returned with removed, damaged or tampered labels (including serial number of product) or any alterations (including the unauthorized removal of any component or external cover).

Loss and Damage

Loss & damage: Zepp Clarity Pixie offers a one-time (1x) replacement for each Zepp Clarity hearing system ("two hearing aids and one charging case") that is lost or damaged during the warranty period, for a fee (stated and updated at clarity.zepp.com). Devices damaged from improper use or care will not be replaced.

How to submit request for repair: Call (855) 619-4327 and we will be happy to assist.

Customer support can also be accessed within the Clarity App.